




Picture 1. Cooling of the sensor of digital thermometer with the piece of ice before its contact with the skin surface.

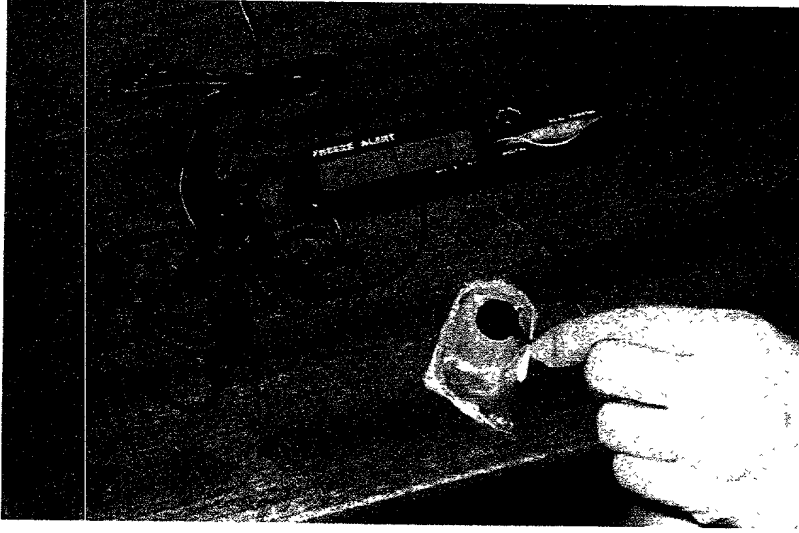


Picture 2. Application of cooled digital thermometer as cold stimuli and measuring device at the same time.

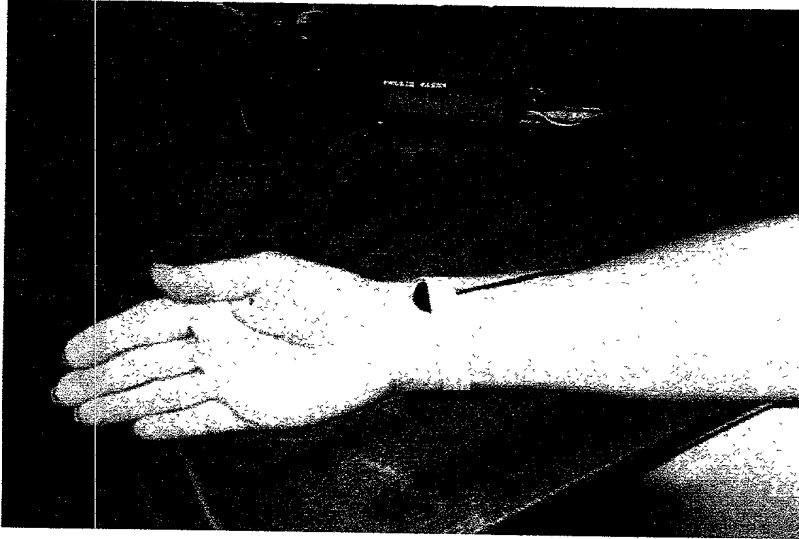

[Handwritten signature]

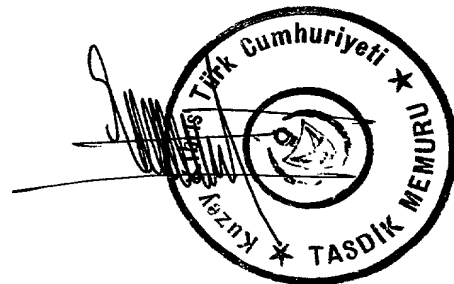

United States Patent & Trademark Office
Office of Initial Patent Examination -- Scanning Division

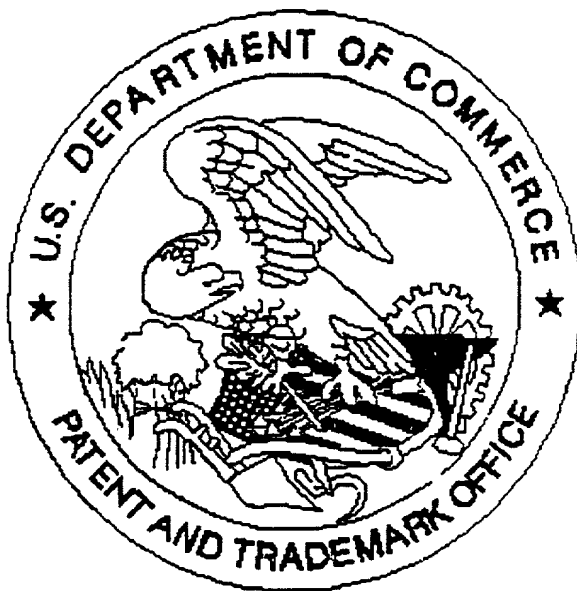

Application deficiencies found during scanning:

☐ Page(s) _____ of _____ were not present
for scanning. (Document title)

☐ Page(s) _____ of _____ were not present
for scanning. (Document title)

☒ Scanned copy is best available. *photographs are very dark.*